

FIG. 2

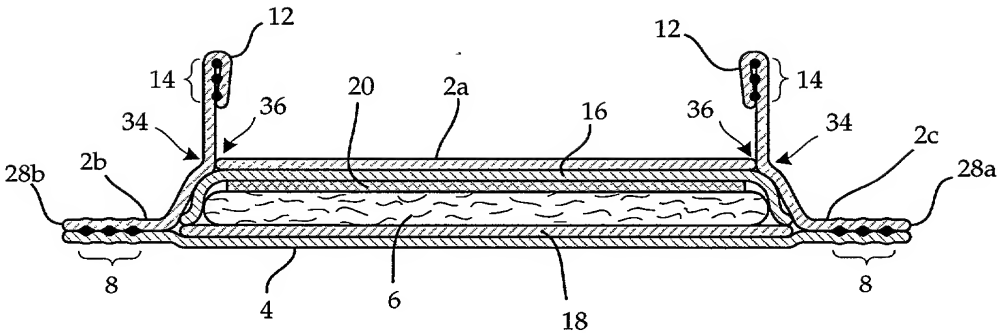


FIG. 3

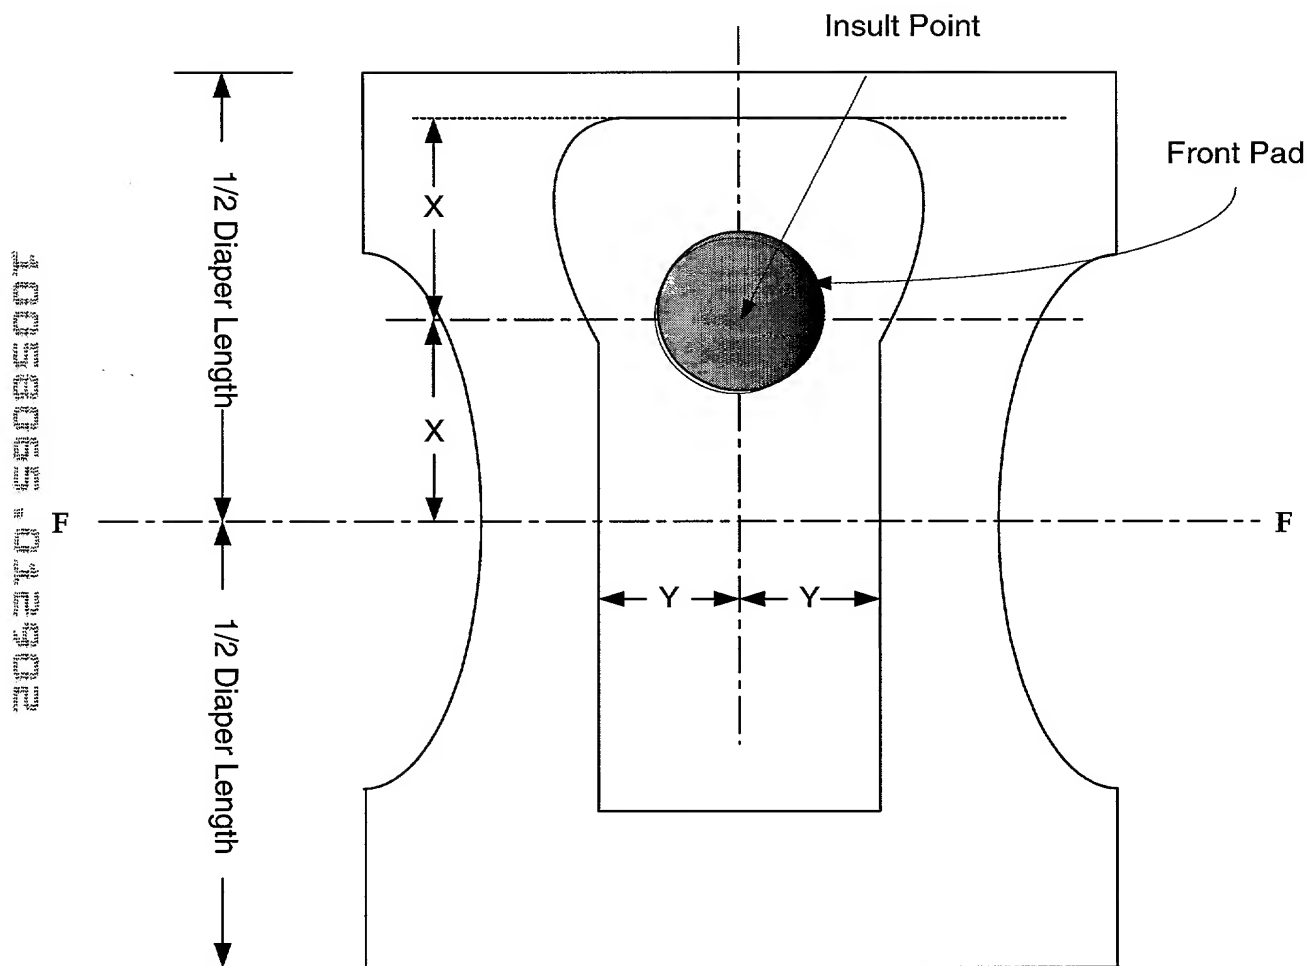


FIG. 4


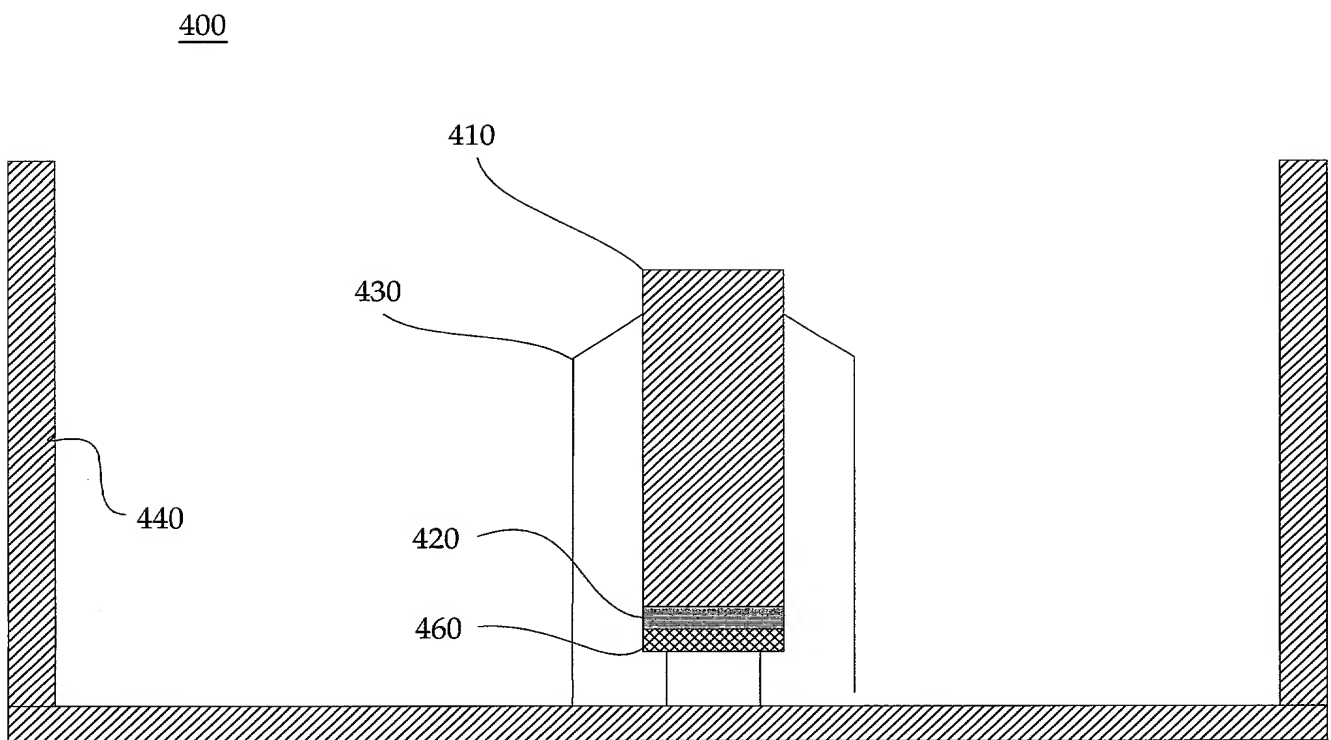


FIG. 5

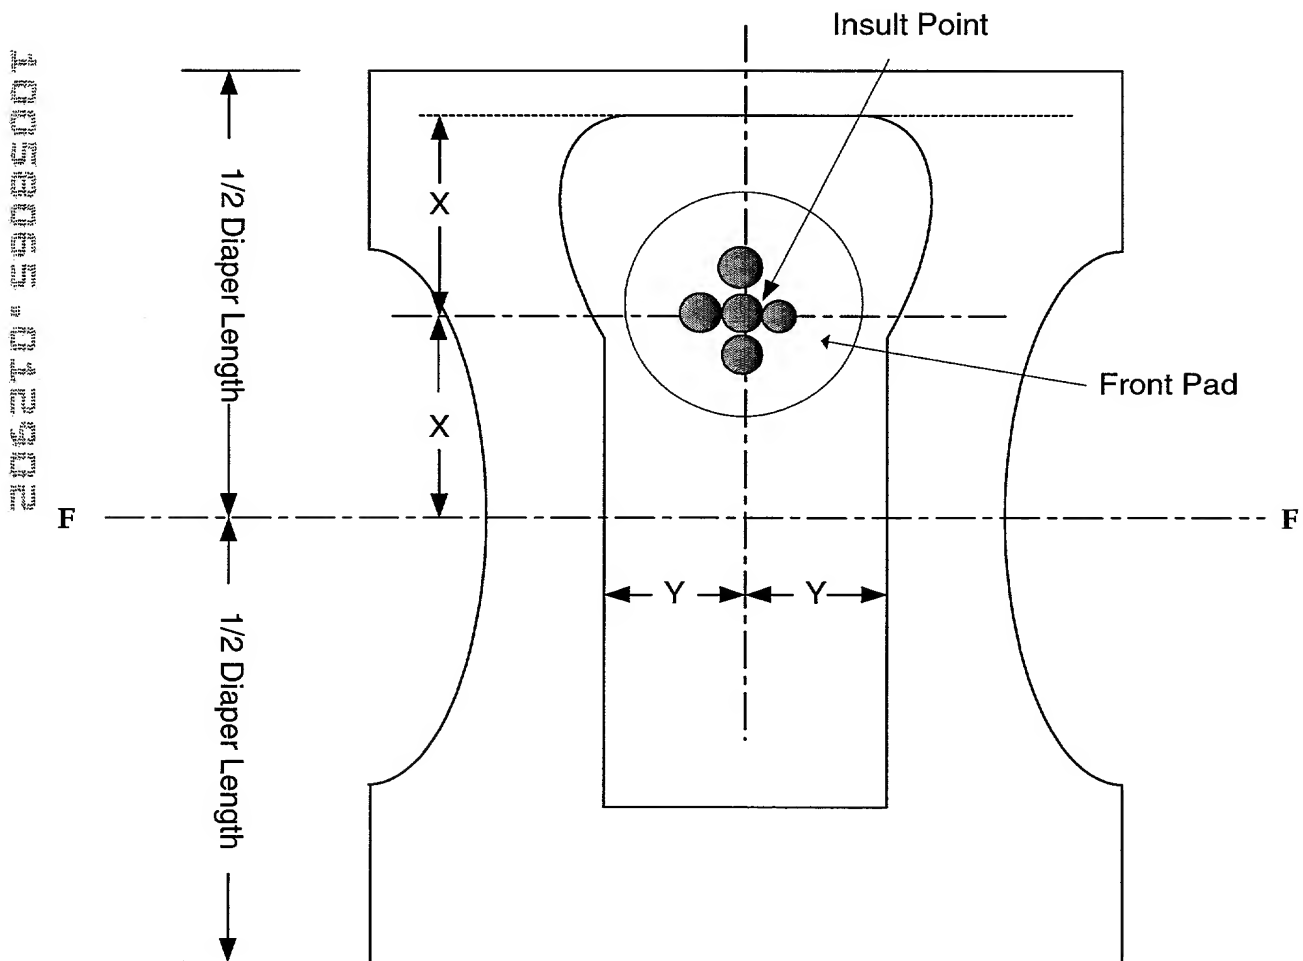

TOTAL FRONT PAD CAPACITY v. Urine Leakage (1.0% NaCl Solution, 10 minutes exposure, 0.5 psi restraining pressure)

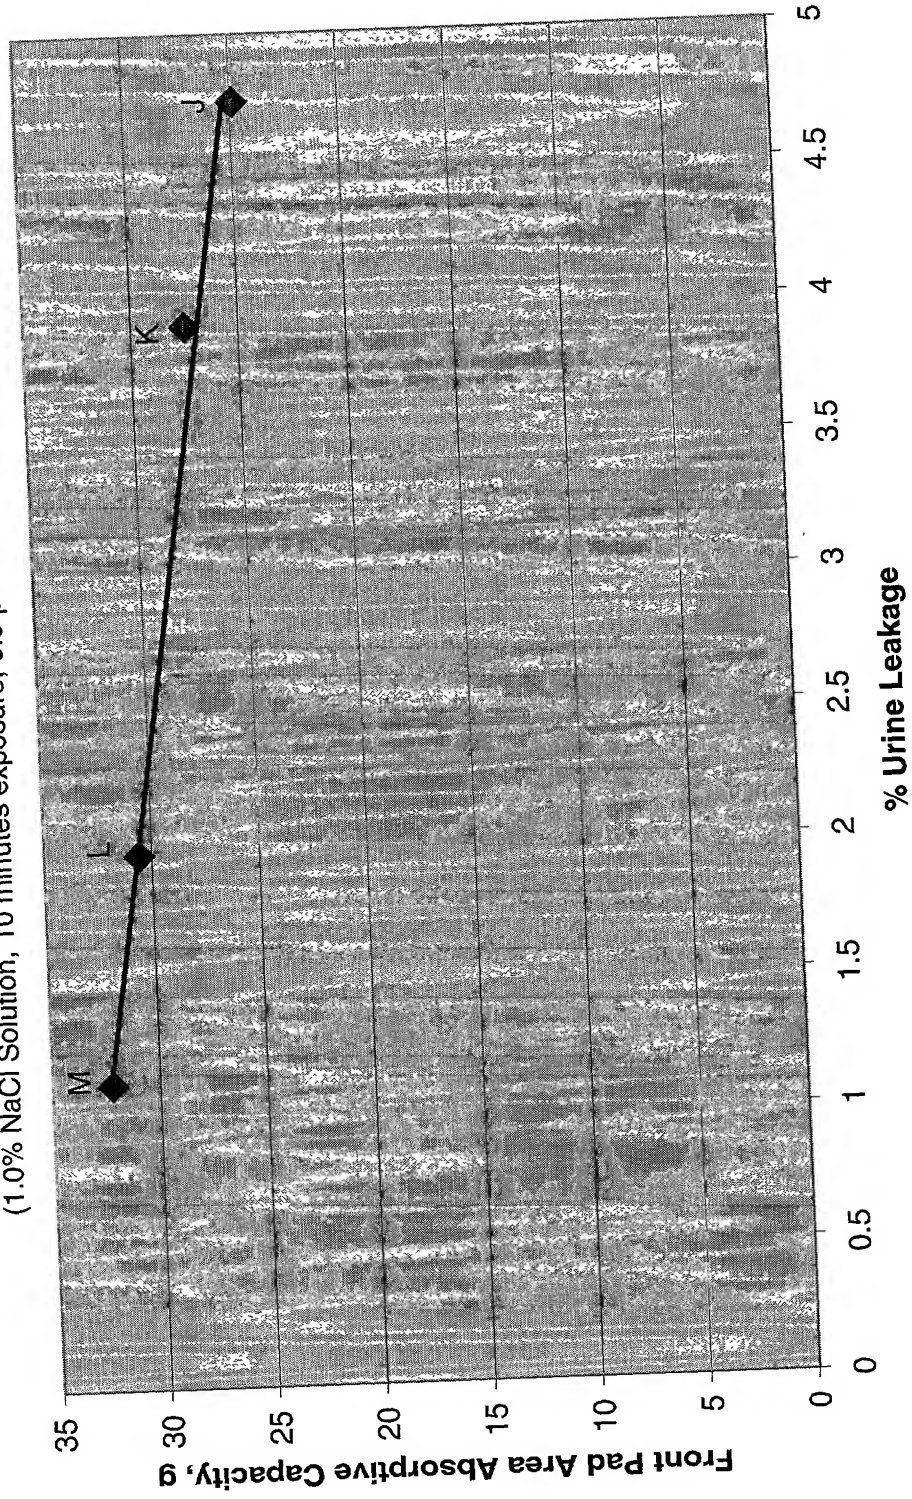


FIG. 6